

# Alcotest 7110 Calibration Record

**Equipment**

Alcotest 7110 MKIII-C  
Serial No.: ARWF-0382  
Location: WEST WINDSOR POLICE  
Calibration File No.: 01278 Calib. Date: 12/09/2015 Calib. No.: 00036  
Certification File No.: 01223 Cert. Date: 06/10/2015 Cert. No.: 00022  
Linearity File No.: 01224 Lin. Date: 06/10/2015 Lin. No.: 00022  
Solution File No.: 01277 Soln. Date: 12/03/2015 Soln. No.: 00188  
Sequential File No.: 01278 File Date: 12/09/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0364  
Control Solution %: 0.100% Expires: 08/17/2017  
Solution Control Lot: 15H143 Bottle No.: 0383

**Coordinator**

Last Name: GONCALVES First Name: MICHELLE MI: L  
Signature: Sgt. Michelle Goncalves #6040 Badge No.: 6040  
Date: 12/09/2015

\*Black Key Temperature Probe Serial.....# DD HHP2-055 (MA)  
\*Digital NIST Temperature Measuring System Serial.....# 150649677 (MG)

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWF-0382  
Location: WEST WINDSOR POLICE  
Calibration File No.: 01278 Calib. Date: 12/09/2015 Calib. No.: 00036  
Certification File No.: 01279 Cert. Date: 12/09/2015 Cert. No.: 00023  
Linearity File No.: 01224 Lin. Date: 06/10/2015 Lin. No.: 00022  
Solution File No.: 01277 Soln. Date: 12/03/2015 Soln. No.: 00188  
Sequential File No.: 01279 File Date: 12/09/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0364  
Control Solution %: 0.100% Expires: 08/17/2017  
Solution Control Lot: 15H143 Bottle No.: 0383

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:24S		
Control 1 EC	0.100%	10:25S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:25S		
Control 2 EC	0.100%	10:26S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:27S		
Control 3 EC	0.101%	10:27S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:28S		

All tests within acceptable tolerance.

### Coordinator

Last Name: GONCALVES First Name: MICHELLE MI: L

Signature: Sgt. Michelle Goncalves #6040 Badge No.: 6040  
Date: 12/09/2015

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWF-0382		
Location:	WEST WINDSOR POLICE				
Calibration File No.:	01278	Calib. Date:	12/09/2015	Calib. No.:	00036
Certification File No.:	01279	Cert. Date:	12/09/2015	Cert. No.:	00023
Linearity File No.:	01280	Lin. Date:	12/09/2015	Lin. No.:	00023
Solution File No.:	01277	Soln. Date:	12/03/2015	Soln. No.:	00188
Sequential File No.:	01280	File Date:	12/09/2015		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDMK S3-0003
Control Solution %:	0.040%			Expires:	08/11/2017
Solution Control Lot:	15H141			Bottle No.:	0023
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXD S3-0193
Control Solution %:	0.080%			Expires:	08/13/2017
Solution Control Lot:	15H142			Bottle No.:	0725
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDCN-0052
Control Solution %:	0.160%			Expires:	08/19/2017
Solution Control Lot:	15H144			Bottle No.:	0975

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:38S		
Control 1 EC	0.041%	10:38S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.041%	10:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:39S		
Control 2 EC	0.041%	10:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.041%	10:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41S		
Control 3 EC	0.082%	10:42S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.082%	10:42S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43S		
Control 4 EC	0.082%	10:44S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.082%	10:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:45S		
Control 5 EC	0.164%	10:45S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.164%	10:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47S		
Control 6 EC	0.164%	10:47S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.164%	10:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:48S		

All tests within acceptable tolerance.

### Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature:



Badge No.: 6040

Date: 12/09/2015



**Dräger**

**Alcotest® 7110 MKIII-C**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

12-3-15

SERIAL NUMBER:

ARWF-0382

Draeger Safety Diagnostics, Inc.

BC



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Dräger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDWJ33-0364

Certification Date

4-30-15

Technician

BC

Re-Certification Due Date

4-30-16

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe, within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWA Pa-215

Certification date:

4-24-15

Next Certification due:

4-24-16

Probe Value

107

**Dräger Safety Diagnostics, Inc.**  
Technical Service Department

BC



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL

DEPARTMENT OF LAW AND PUBLIC SAFETY

DIVISION OF STATE POLICE

POST OFFICE BOX 7068

WEST TRENTON, NJ 08628-0068

(609) 882-2000

CHRIS CHRISTIE  
Governor

KIM GUADAGNO  
Lt. Governor

JOHN J. HOFFMAN  
Acting Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

**MANUFACTURER:** Draeger Safety, Inc.

**ANALYSIS DATE:** 5/6/2015

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 15D138

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1203 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 13, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.  
Research Scientist  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 14<sup>th</sup> day of May, 2015.

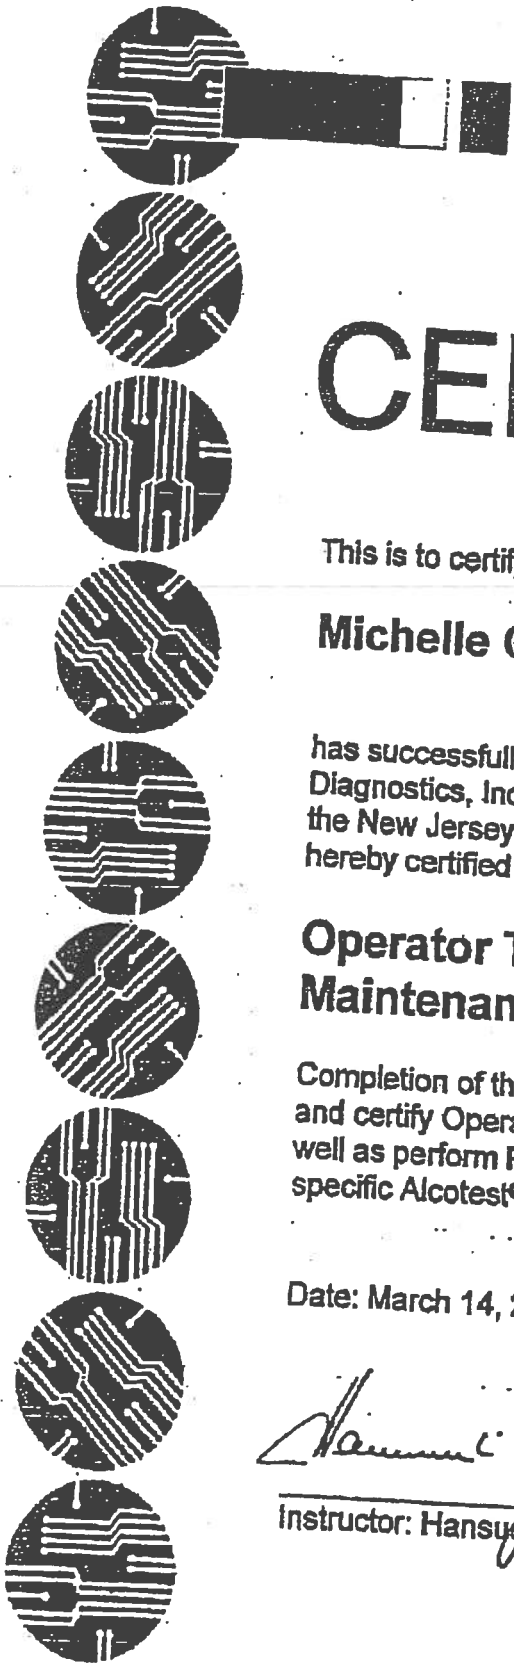
Notary  
**MARY ELIZABETH MCLAUGHLIN**  
ID # 2052190  
NOTARY PUBLIC  
STATE OF NEW JERSEY  
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable





# CERTIFICATE

This is to certify that

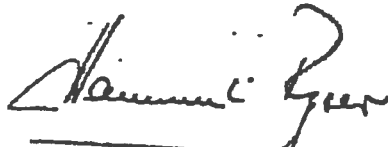
**Michelle Goncalves**

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and  
Maintenance Technician**

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: March 14, 2012

  
\_\_\_\_\_  
Instructor: Hansueli Ryser

**Dräger**





Calibration  
Certificate No. 1750.01

**Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001**



**Cert. No.: 4000-7019767**

**Traceable® Certificate of Calibration for Digital Thermometer**

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087

**Instrument Identification:**

Model: 61220-601      S/N: 150649677      Manufacturer: Control Company

**Standards/Equipment:**

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-256	B01375		
Temperature Probe	128	4/02/16	15-A0P2S-40-1
Thermistor Module	A17118	3/03/16	1000371058
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17118	3/03/16	1000371058
Temperature Probe	3039	4/02/16	15-A0P2S-20-1
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A27129	11/04/15	1000365407
Temperature Probe	5202	11/19/16	6-CV9Y2-1-1
Temperature Calibration Bath TC-309	B3A444		
Thermistor Module	A27129	11/04/15	1000365407
Temperature Probe	5267	11/19/16	6-CV9Y0-1-1

**Certificate Information:**

Technician: 68      Procedure: CAL-06      Cal Date: 8/31/15      Due Date: 8/31/17  
 Test Conditions: 23.0°C      47.0 %RH      1017 mBar

**Calibration Data: (New Instrument)**

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.001	0.000	Y	-0.049	0.051	0.013	3.8:1
°C		N.A.		25.000	25.001	Y	24.950	25.050	0.014	3.6:1
°C		N.A.		50.004	50.000	Y	49.954	50.054	0.014	3.6:1
°C		N.A.		100.002	99.999	Y	99.952	100.052	0.014	3.6:1

**This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.**

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

*Nicol Rodriguez*  
Nicol Rodriguez, Quality Manager

*Aaron Judice*  
Aaron Judice, Technical Manager

**Maintaining Accuracy:**

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

**Recalibration:**

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

**CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA**  
**Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com**

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
 Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-RVA.  
 International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**Michelle L. Gonçalves**  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C** A METHOD TO DETERMINE INTOXICATION, GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 15th DAY OF December

TWO THOUSAND AND Eleven

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**Michelle Gonçalves**  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE **Breath Test Coordinator/Instructor** A METHOD TO DETERMINE INTOXICATION, GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 23rd DAY OF March

TWO THOUSAND AND Twelve

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 12-3-13	GCFA	Wm Lewis
2. 9/17/15	GCFA	Adrian Garcia
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 03/10)

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 02/12)



CHRIS CHRISTIE  
Governor

KIM GUADAGNO  
Lieutenant Governor

*State of New Jersey*  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF CRIMINAL JUSTICE  
PO BOX 085  
TRENTON, NJ 08625-0085  
TELEPHONE: (609) 984-6500

JEFFREY S. CHIESA  
Attorney General

STEPHEN J. TAYLOR  
Director

March 23, 2012

Col. Joseph R. Fuentes, Superintendent  
Division of State Police  
Division Headquarters  
P.O. Box 7068  
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification -  
Detective I Michelle L. Goncalves #6040

Dear Col. Fuentes:

Pursuant to the provisions of *N.J.A.C. 13:51-2.1* (b) and (c), as adopted and promulgated under the provisions of *N.J.S.A. 39:4-50.3*, *39:3-10.25* and *12:7-56*, I hereby approve Detective I Michelle L. Goncalves #6040, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,

Jeffrey S. Chiesa  
Attorney General

- c. Detective I Michelle L. Goncalves, Alcohol/Drug Test Unit, Division of State Police  
DSFC Patrick Guilfroy, Unit Head, Alcohol/Drug Test Unit, Division of State Police





**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXDS3 - 0193

Certification Date

9-22-15

Technician

72

Re-Certification Due Date

9-22-16

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDHHP2-055

Certification date:

10-30-15

Next Certification due:

10-30-16

Probe Value

104

Draeger Safety Diagnostics, Inc.  
Technical Service Department

BC



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDMKS3-0003

Certification Date

Technician

Re-Certification Due Date

10-30-15

72

10-30-16



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDCN-0052

Certification Date

Technician

Re-Certification Due Date

10-30-15

72

10-30-16



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

JOHN J. HOFFMAN
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/14/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15H143

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1198 to 0.1226 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 17, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaouie]

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18th day of September, 2015.

[Handwritten signature of Mary Elizabeth McLaughlin]
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON, NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

KIM GUADAGNO  
 Lt. Governor

JOHN J. HOFFMAN  
 Acting Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 9/10/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15H141

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0478 to 0.0487 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 11, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.  
 Research Scientist  
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 11<sup>th</sup> day of September, 2015.

Notary **MARY ELIZABETH MCLAUGHLIN**

ID # 2052190  
 NOTARY PUBLIC  
 STATE OF NEW JERSEY  
 My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON, NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

KIM GUADAGNO  
 Lt. Governor

JOHN J. HOFFMAN  
 Acting Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

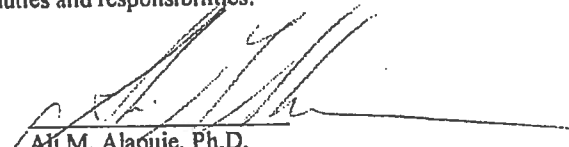
ANALYSIS DATE: 9/17/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15H142


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0959 to 0.0967 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 13, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
 Ali M. Alaoui, Ph.D.  
 Research Scientist  
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18<sup>th</sup> day of September, 2015.

  
 Notary  
**MARY ELIZABETH MCLAUGHLIN**  
 ID # 2052190  
 NOTARY PUBLIC  
 STATE OF NEW JERSEY  
 My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable







State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON, NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

KIM GUADAGNO  
 Lt. Governor

JOHN J. HOFFMAN  
 Acting Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

**MANUFACTURER:** Draeger Safety, Inc.


**ANALYSIS DATE:** 9/17/2015

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 15H144


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1936 to 0.1952 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 19, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
 Ali M. Alaouie, Ph.D.  
 Research Scientist  
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18 day of September, 2015.

  
 Notary  
**JOHN R LEAVER**  
 ID # 2207138  
 NOTARY PUBLIC  
 STATE OF NEW JERSEY  
 My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable

