

# Calibrating Unit

## New Standard Solution Report

|                                |                       |                     |              |
|--------------------------------|-----------------------|---------------------|--------------|
| <b>Equipment</b>               | Alcotest 7110 MKIII-C | Serial No.:         | ARWF-0382    |
| <b>Location:</b>               | WEST WINDSOR POLICE   |                     |              |
| <b>Calibration File No.:</b>   | 01074                 | <b>Calib. Date:</b> | 02/06/2014   |
| <b>Certification File No.:</b> | 01075                 | <b>Cert. No.:</b>   | 00031        |
| <b>Linearity File No.:</b>     | 01076                 | <b>Cert. Date:</b>  | 02/06/2014   |
| <b>Solution File No.:</b>      | 01096                 | <b>Lin. Date:</b>   | 02/06/2014   |
| <b>Sequential File No.:</b>    | 01096                 | <b>Lin. No.:</b>    | 00019        |
|                                |                       | <b>Soln. Date:</b>  | 04/03/2014   |
|                                |                       | <b>Soln. No.:</b>   | 00153        |
|                                |                       | <b>File Date:</b>   | 04/03/2014   |
| <b>Calibrating Unit:</b>       | WET                   | <b>Model No.:</b>   | CU-34        |
| <b>Control Solution %:</b>     | 0.100%                | <b>Serial No.:</b>  | DDWJ S3-0364 |
| <b>Solution Control Lot:</b>   | 13G115                | <b>Expires:</b>     | 07/18/2015   |
|                                |                       | <b>Bottle No.:</b>  | 0998         |

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 10:00S        |                               |                           |
| Control 1 EC      | -.---%         | 10:01S        | 30.2°C                        | SIMULATOR TEMP. ERROR     |
| Control 1 IR      | -.---%         | 10:01S        | 30.2°C                        | SIMULATOR TEMP. ERROR     |
| Ambient Air Blank | -.---%         | --:--         |                               |                           |
| Control 2 EC      | -.---%         | --:--         | N/A                           |                           |
| Control 2 IR      | -.---%         | --:--         | N/A                           |                           |
| Ambient Air Blank | -.---%         | --:--         |                               |                           |
| Control 3 EC      | -.---%         | --:--         | N/A                           |                           |
| Control 3 IR      | -.---%         | --:--         | N/A                           |                           |
| Ambient Air Blank | -.---%         | --:--         |                               |                           |

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MCMAHON

First Name: MICHAEL

MI: J

Signature: \_\_\_\_\_

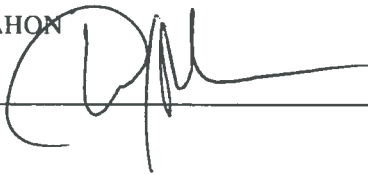

Badge No.: 80

Date: 04/03/2014

# Calibrating Unit

## New Standard Solution Report

|                         |                       |              |              |
|-------------------------|-----------------------|--------------|--------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C | Serial No.:  | ARWF-0382    |
| Location:               | WEST WINDSOR POLICE   |              |              |
| Calibration File No.:   | 01074                 | Calib. Date: | 02/06/2014   |
| Certification File No.: | 01075                 | Cert. No.:   | 00031        |
| Linearity File No.:     | 01076                 | Cert. Date:  | 02/06/2014   |
| Solution File No.:      | 01097                 | Lin. No.:    | 00019        |
| Sequential File No.:    | 01097                 | Lin. Date:   | 02/06/2014   |
|                         |                       | Soln. No.:   | 00154        |
|                         |                       | Soln. Date:  | 04/03/2014   |
|                         |                       | File Date:   | 04/03/2014   |
| <br>                    |                       |              |              |
| Calibrating Unit:       | WET                   | Model No.:   | CU-34        |
| Control Solution %:     | 0.100%                | Serial No.:  | DDWJ S3-0364 |
| Solution Control Lot:   | 13G115                | Expires:     | 07/18/2015   |
|                         |                       | Bottle No.:  | 0997         |

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 12:18S        |                               |                           |
| Control 1 EC      | 0.100%         | 12:18S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.100%         | 12:18S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 12:19S        |                               |                           |
| Control 2 EC      | 0.099%         | 12:20S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.100%         | 12:20S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 12:20S        |                               |                           |
| Control 3 EC      | 0.099%         | 12:21S        | 33.9°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.100%         | 12:21S        | 33.9°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 12:22S        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MCMAHON

First Name: MICHAEL

MI: J

Signature: \_\_\_\_\_



Badge No.: 80

Date: 04/03/2014